
Data sheet
L-9517-9426-04-B

RENISHAW
apply innovation™

TONiC™ UHV encoder system

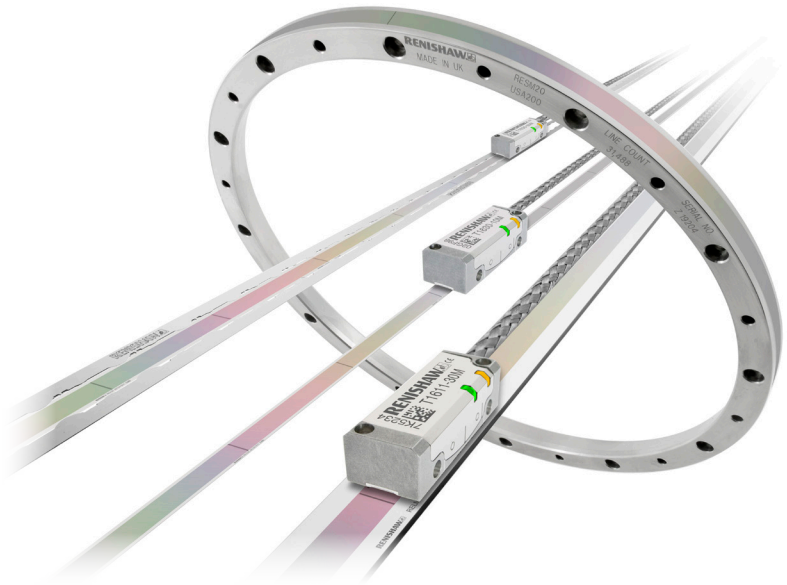

The TONiC UHV encoder offers all the benefits of the established TONiC linear and rotary encoder systems in a readhead that has been designed and constructed using ultra-high vacuum compatible materials and processes.

The TONiC UHV readhead is compatible with a wide range of linear and rotary scales with bi-directional optical IN-TRAC™ reference marks.

For ultimate reliability and high immunity to optical degradation,TONiC UHV readheads incorporate Renishaw's market-proven filtering optics, tuned for even lower noise (jitter), further enhanced by dynamic signal processing including Auto Gain Control (AGC) and Auto Offset Control (AOC). The result is ultra-low sub-divisional error (SDE) giving smoother velocity control for improved scanning performance and increased positional stability.


TONiC UHV readheads also feature a detachable analogue or digital interface in the form of a robust, convenient connector that can be located up to 10 m from the readhead. The interface offers digital interpolation to 1 nm resolution, with clocked outputs for optimised speed performance at all resolutions for industry-standard controllers.



The readhead carries an integral set-up LED that enables quick and easy installation. All of these readheads are supplied with an RFI-screened UHV-compatible cable as standard.

- **Clean RGA**
- **Low outgassing rates**
- **High bake-out temperature of 120 °C**
- **Low power consumption readheads**
- **Non-contact open optical system**
- **Detachable analogue or digital connector with integral interpolation to 1 nm resolution (0.00075 arc seconds)**
- **Resolution to 1 nm**
- **Dynamic signal processing provides ultra-low SDE of typically ±30 nm**
- **Auto Gain Control (AGC) ensures constant signal strength for long-term reliability**
- **Compatible with a wide range of linear and rotary scales with customer selectable IN-TRAC auto-phase optical reference mark (datum)**

Compatible scales

Linear scales

	RTLC20-S	RTLC20/FASTRACK™	RKLC20-S
	Self-adhesive mounted stainless-steel tape scale	**Stainless-steel tape scale and self-adhesive mounted carrier**	**Self-adhesive mounted stainless-steel tape scale**
			
Form (height × width)	0.4 mm × 8 mm including adhesive	RTLC20 scale: 0.2 mm × 8 mm FASTRACK carrier: 0.4 mm × 18 mm including adhesive	0.15 mm × 6 mm including adhesive
Accuracy (includes slope and linearity)	±5 µm/m	±5 µm/m	±5 µm/m
Linearity (figures achievable with two-point error correction)	±2.5 µm/m	±2.5 µm/m	±2.5 µm/m
Maximum length	10 m [1] (> 10 m available on request)	10 m (> 10 m available on request)	20 m (> 20 m available on request)
Coefficient of thermal expansion (at 20 °C)	10.1 ±0.2 µm/m/°C	10.1 ±0.2 µm/m/°C	Matches that of substrate material when scale ends rigidly fixed [2]

	RSLM20	RELM20
	Self-adhesive or clip/clamp mounted stainless-steel spar scale	**Self-adhesive or clip/clamp mounted low-expansion ZeroMet™ spar scale**
		
Form (height × width)	1.5 mm × 14.9 mm	1.6 mm × 14.9 mm
Accuracy (includes slope and linearity)	±4 µm (total accuracy over a complete 5 m length)	±1 µm (total accuracy up to 1 m)
Linearity (figures achievable with two-point error correction)	N/A	N/A
Maximum length	5 m	1.7 m
Coefficient of thermal expansion (at 20 °C)	10.1 ±0.2 µm/m/°C	0.75 ±0.35 µm/m/°C

NOTE: For more information about the scales refer to the relevant scale data sheet which can be downloaded from www.renishaw.com/tonicdownloads.

[1] For RTLC20-S axis lengths > 2 m, FASTRACK with RTLC20 is recommended.

[2] Scale mastering is not guaranteed after system bake-out.

Rotary scales

	RESM20	REXM20
	Stainless-steel ring	**Ultra-high accuracy stainless-steel ring**
		
Accuracy	±1.9 arc second (typical installed accuracy for a 550 mm diameter RESM20 ring) [1]	±1 arc second [2] (total installed accuracy for a 417 mm diameter REXM20 ring)
Ring diameters	52 mm to 550 mm	52 mm to 417 mm
Coefficient of thermal expansion (at 20 °C)	15.5 ±0.5 µm/m/°C	15.5 ±0.5 µm/m/°C


NOTE: For more information about the scales refer to the relevant scale data sheet which can be downloaded from www.renishaw.com/tonicdownloads.

[1] "Typical" installations are a result of graduation and installation errors combining and, to some magnitude, cancelling.

[2] When using two readheads and an additional DSi interface.

TONiC readhead installation drawing (on RTLC20-S scale)

Dimensions and tolerances in mm

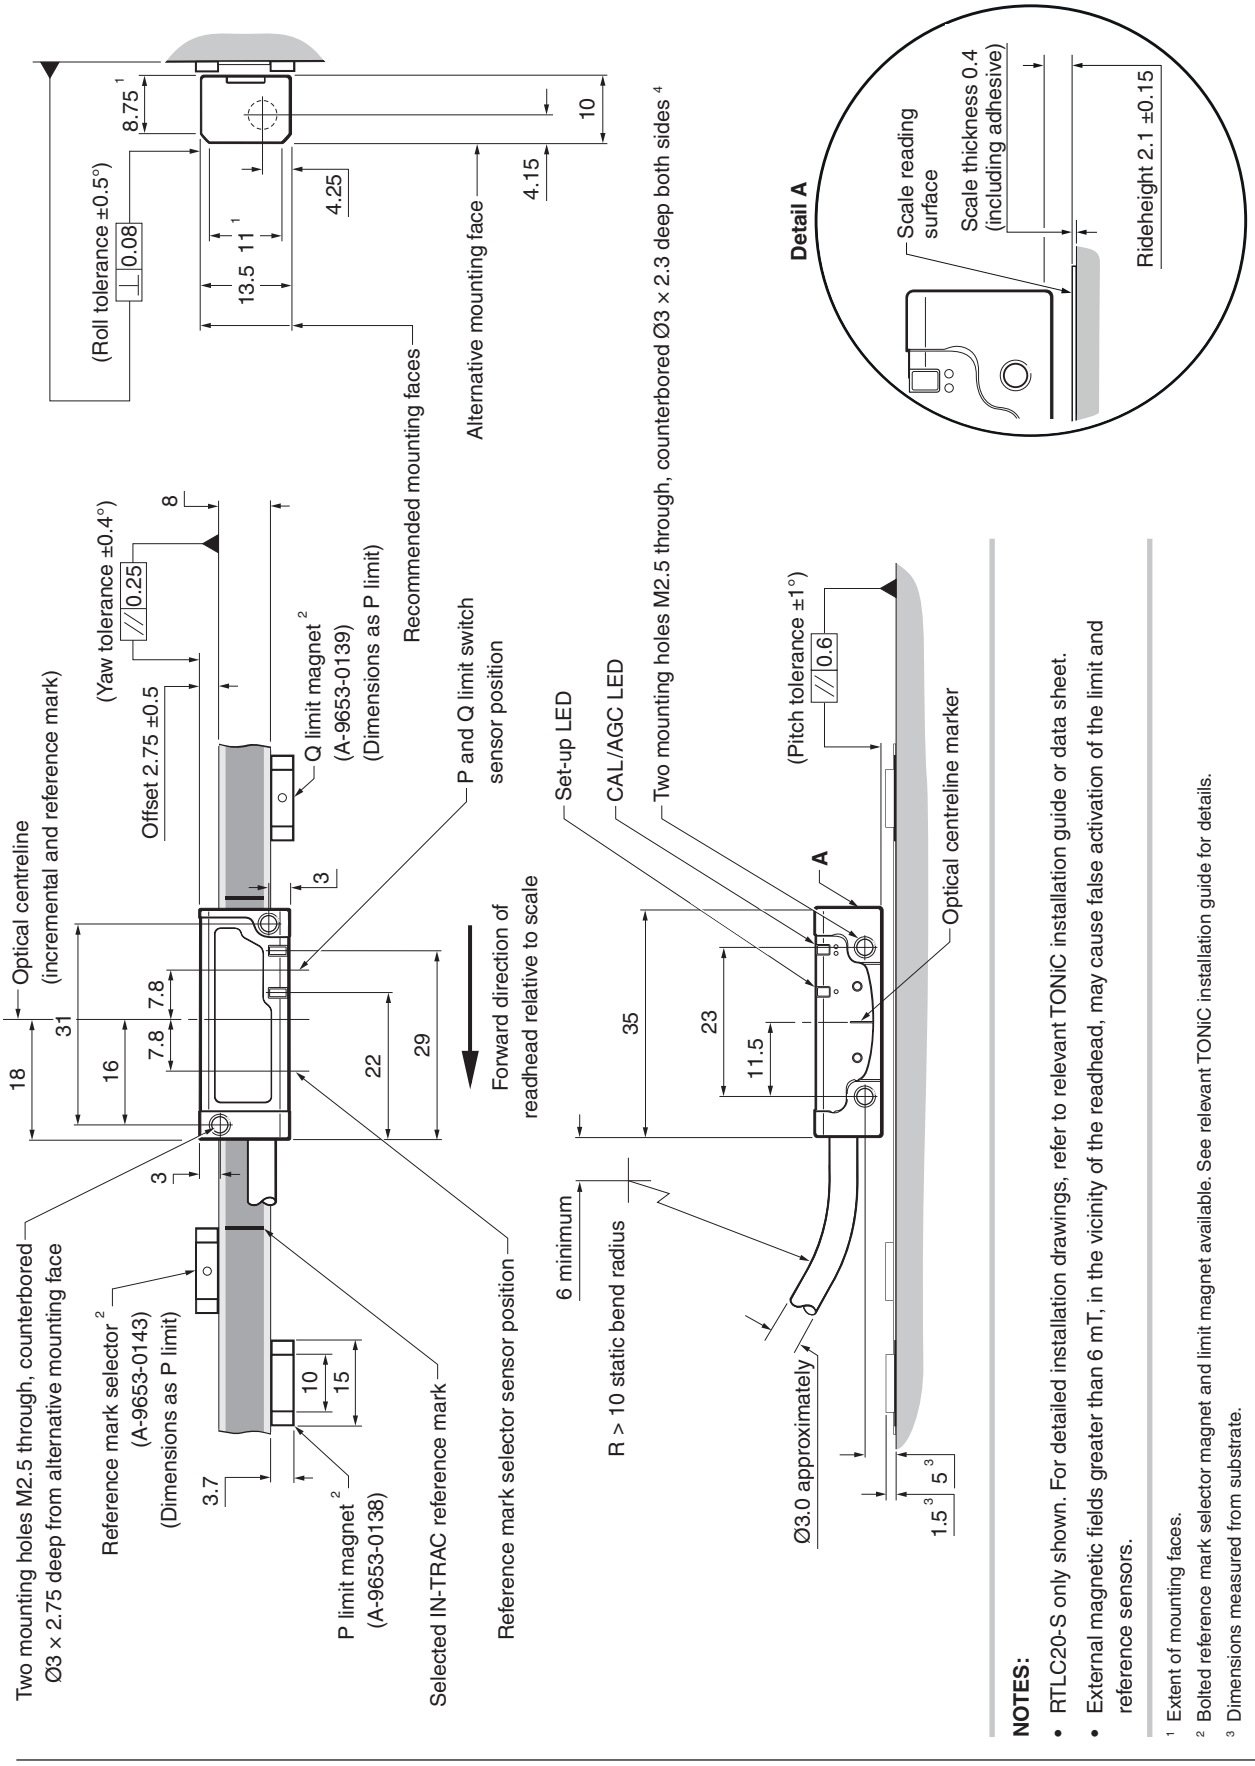

NOTES:

- RTLC20-S only shown. For detailed installation drawings, refer to relevant TONiC installation guide or data sheet.
- External magnetic fields greater than 6 mT, in the vicinity of the readhead, may cause false activation of the limit and reference sensors.

[1] Extent of mounting faces.


[2] Bolted reference mark selector magnet and limit magnet available. See relevant TONiC installation guide for details.

[3] Dimensions measured from substrate.

[4] The recommended thread engagement is 5 min (7.5 including counterbore). The recommended tightening torque is between 0.25 and 0.4 Nm.

TONiC readhead installation drawing (on RESM20 ring)

Dimensions and tolerances in mm

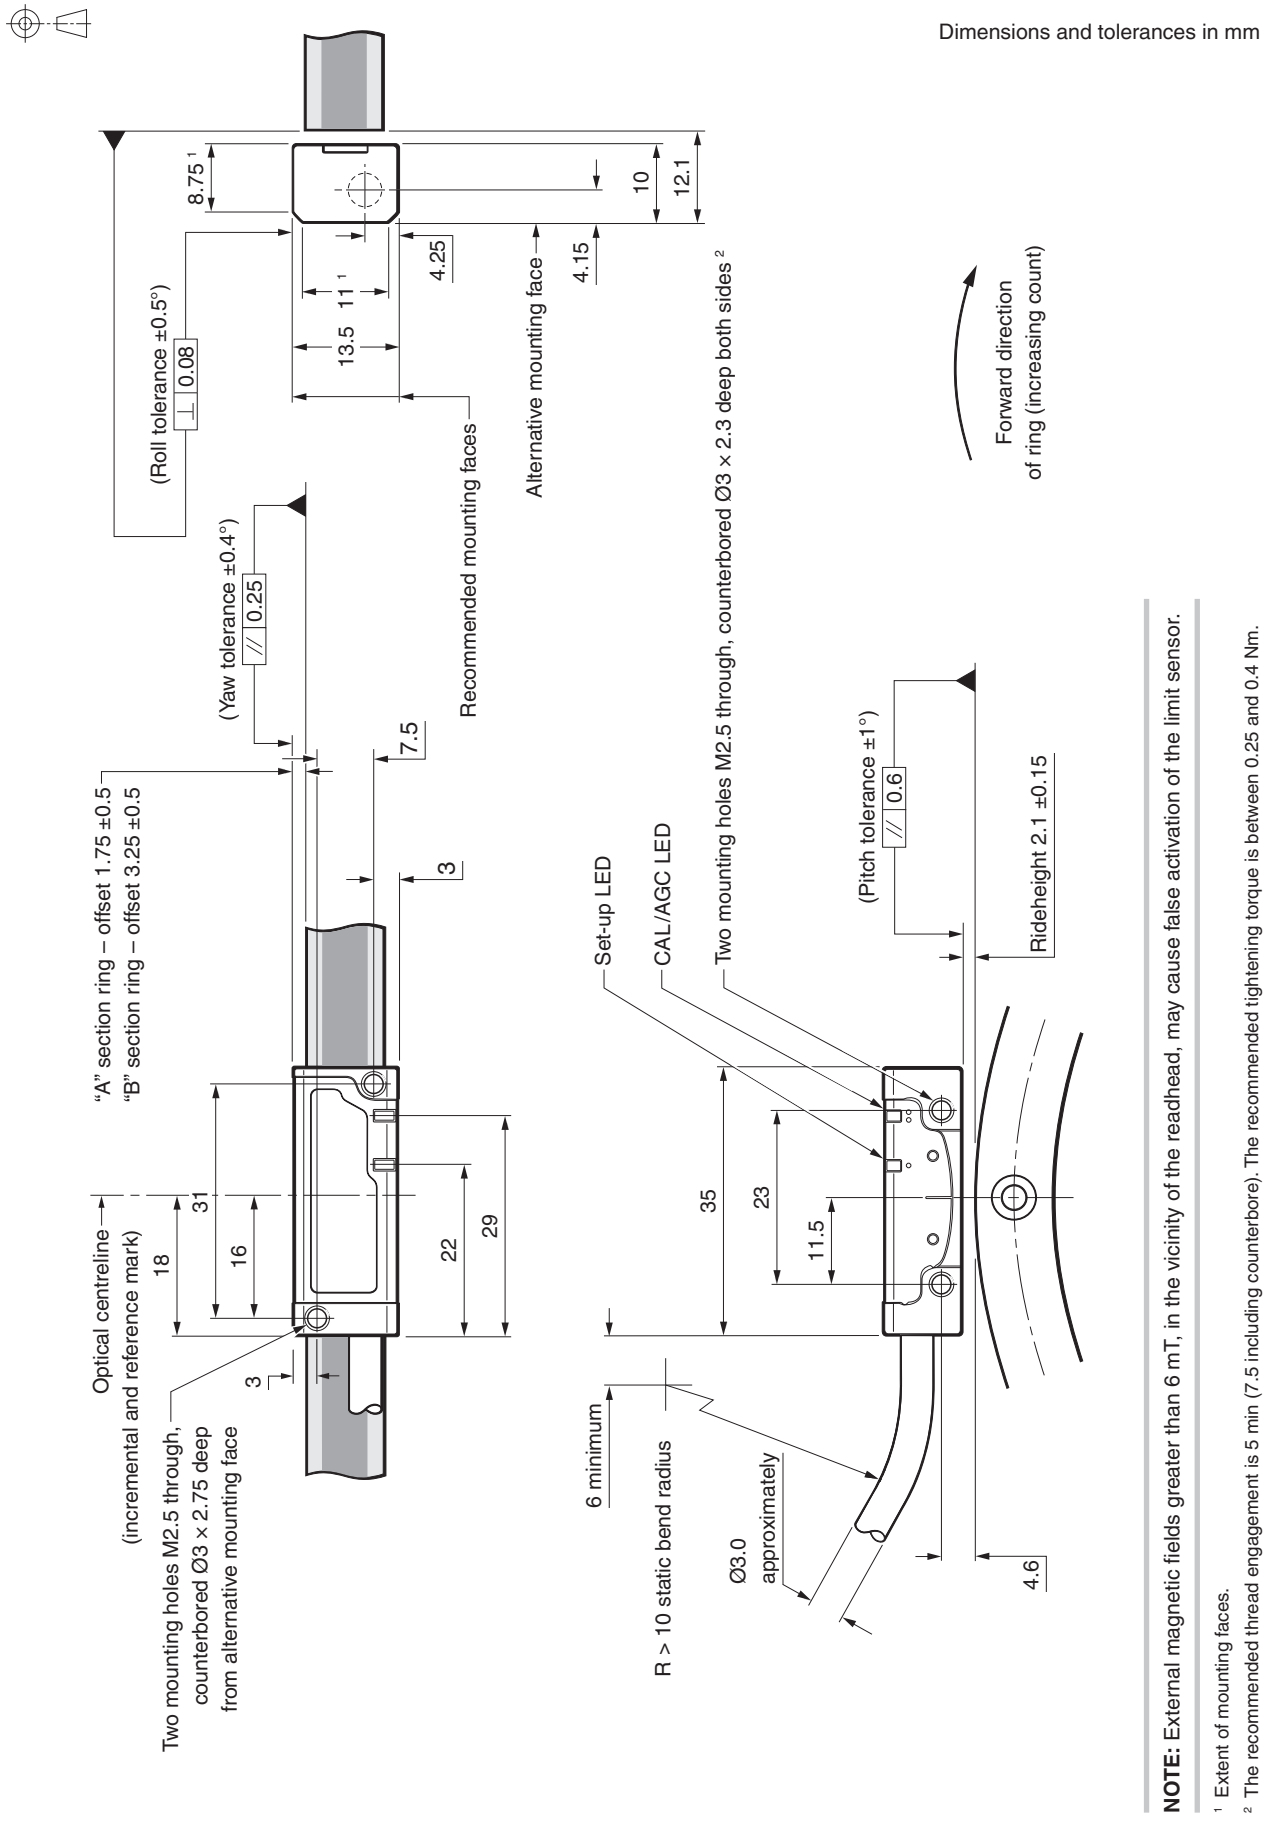


NOTE: External magnetic fields greater than 6 mT, in the vicinity of the readhead, may cause false activation of the limit sensor.


[1] Extent of mounting faces.


[2] The recommended thread engagement is 5 min (7.5 including counterbore). The recommended tightening torque is between 0.25 and 0.4 Nm.

Ti/TD interface dimension drawing

Dimensions and tolerances in mm

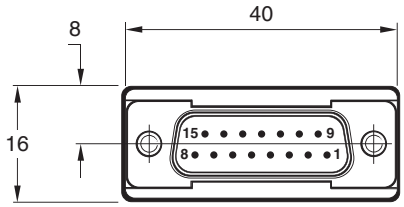

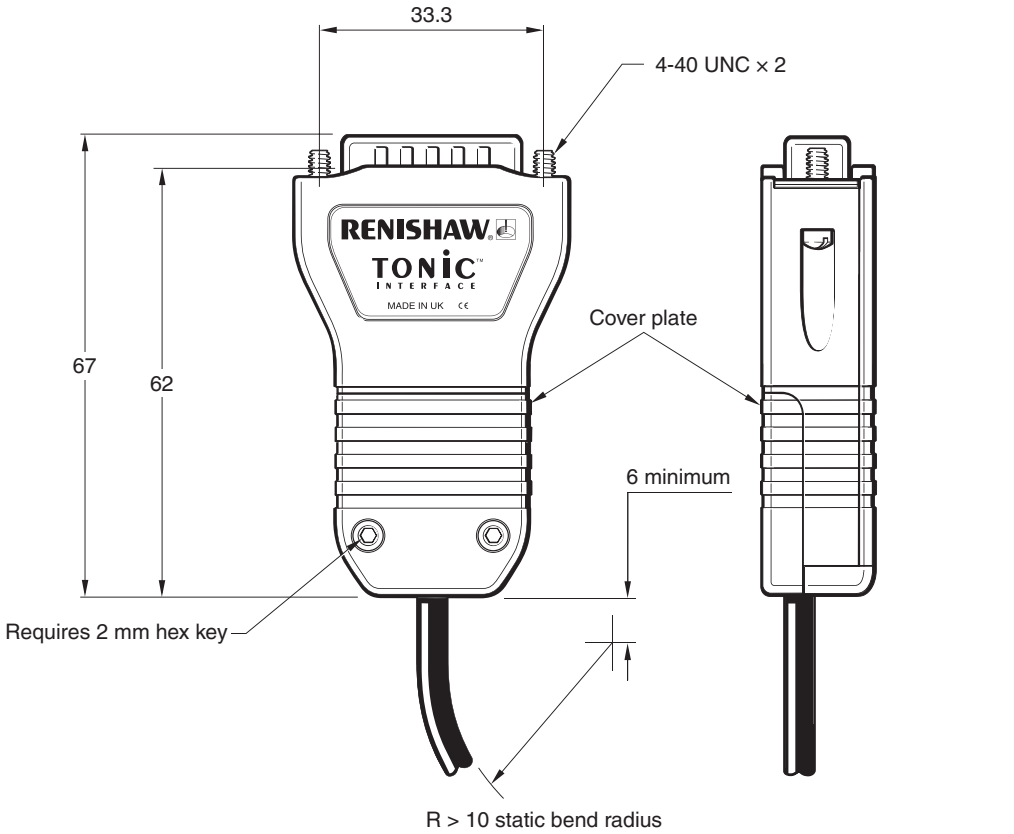

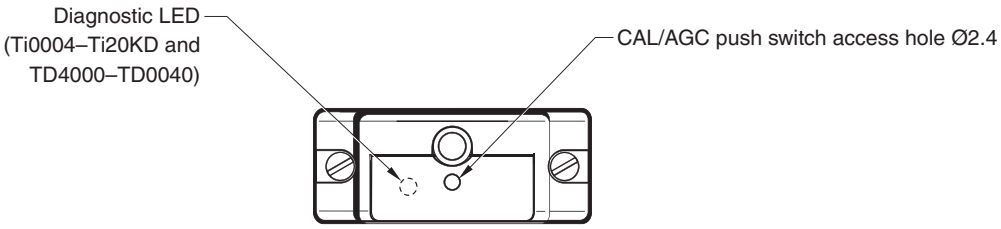

TD dual resolution interface

Allows output to be switched between two resolutions. See TD interface part number section for details of available resolutions.

NOTES:

- It is recommended that movement should be halted before switching resolutions.
- There are no limit outputs.

General specifications

Power supply [1]	5V ±10%	Readhead only < 100 mA T16xx/T26xx with Ti0000 < 100 mA T16xx/T26xx with Ti0004 - Ti20KD or TD4000 - TD0040 < 200 mA For digital outputs, a further 25 mA per channel pair (e.g., A+, A–) will be drawn when terminated with 120R For analogue outputs, a further 20 mA in total will be drawn when terminated with 120R Power from a 5 Vdc supply complying with the requirements for SELV of standard IEC 60950-1
	Ripple	200 mVpp maximum @ frequency up to 500 kHz
Temperature (system)	Storage	–20 °C to +70 °C
	Operating	0 °C to +70 °C
	Bake-out	120 °C
Humidity (system)		95% relative humidity (non-condensing) to IEC 60068-2-78
Sealing	Readhead	IP20
	Interface	IP20
Acceleration (readhead)	Operating	500 m/s², 3 axes
Shock (system)	Operating	500 m/s², 11 ms, ½ sine, 3 axes
Vibration (system)	Operating	Sinusoidal 100 m/s² max @ 55 Hz to 2000 Hz, 3 axes
Mass	Readhead	10 g
	Interface	100 g
	Cable	14 g/m
EMC compliance (system)		IEC 61326-1
Readhead cable		Tinned copper braided single screen. FEP core insulation
Typical sub-divisional error (SDE)		±30 nm

[1] Current consumption figures refer to unterminated systems.

Speed

Clocked output option (MHz)	Maximum speed (m/s)										
	Ti0004 5 µm	Ti0020 1 µm	Ti0040 0.5 µm	Ti0100 0.2 µm	Ti0200 0.1 µm	Ti0400 50 nm	Ti1000 20 nm	Ti2000 10 nm	Ti4000 5 nm	Ti10KD 2 nm	Ti20KD 1 nm
50	10	10	10	6.48	3.240	1.625	0.648	0.324	0.162	0.065	0.032
40	10	10	10	5.40	2.700	1.350	0.540	0.270	0.135	0.054	0.027
25	10	10	8.10	3.24	1.620	0.810	0.324	0.162	0.081	0.032	0.016
20	10	10	6.75	2.70	1.350	0.670	0.270	0.135	0.068	0.027	0.013
12	10	9	4.50	1.80	0.900	0.450	0.180	0.090	0.045	0.018	0.009
10	10	8.10	4.05	1.62	0.810	0.400	0.162	0.081	0.041	0.016	0.0081
08	10	6.48	3.24	1.29	0.648	0.324	0.130	0.065	0.032	0.013	0.0065
06	10	4.50	2.25	0.90	0.450	0.225	0.090	0.045	0.023	0.009	0.0045
04	10	3.37	1.68	0.67	0.338	0.169	0.068	0.034	0.017	0.0068	0.0034
01	4.2	0.84	0.42	0.16	0.084	0.042	0.017	0.008	0.004	0.0017	0.0008
Analogue output	10 (–3 dB)										

NOTE: TD interface maximum speeds are resolution dependent, as defined above.

Angular speed depends on ring diameter – use the following equation to convert to rev/min:

$$\text{Angular speed (rev/min)} = \frac{V \times 1000 \times 60}{\pi D}$$

Where V = maximum linear speed (m/s) and
D = external diameter of RESM20 or REXM20 ring (mm).


Output signals

Digital outputs

			Interface	
			Ti0004 – Ti20KD	TD4000 – TD0040
Function	**Signal**		**Pin**	**Pin**
Power	5 V		7, 8	7, 8
	0 V		2, 9	2, 9
Incremental	A	+	14	14
		–	6	6
	B	+	13	13
		–	5	5
Reference mark	Z	+	12	12
		–	4	4
Limits	P [1]		11	-
	Q		10	-
Set-up	X		1	1
Alarm [2]	E	+	-	11
		–	3	3
Resolution switching [3]	-		-	10
Shield	Inner		-	-
	Outer		Case	Case

Analogue outputs

				Readhead T16xx/26xx	Interface Ti0000
Function		**Signal**		**Colour**	**Pin**
Power		5 V		Brown	4, 5
		0 V		White	12, 13
Incremental	Cosine	V_1	+	Red	9
			–	Blue	1
	Sine	V_2	+	Yellow	10
			–	Green	2
Reference mark		V_0	+	Violet	3
			–	Grey	11
Limits		V_p		Pink	7
		V_q		Black	8
Set-up		V_x		Clear	6
Remote CAL		CAL		Orange	14
Shield		-		Screen	Case



15-pin D-type connector

[1] Becomes alarm (E+) for Ti options E, F, G, H.

[2] The alarm signal can be output as a line-driven signal or 3-state. Please select the preferred option at time of ordering.

[3] On TD interfaces pin 10 should be connected to 0 V to switch to lower resolution.

RGA results


Test schedule

A quadrupole mass spectrometer (AccuQuad 200 RGA), set to 200AMU scan range, was used to collect RGA (residual gas analysis) data and to measure total chamber pressure. After initial conditioning of the system, a background spectrum was recorded together with the total pressure in the test chamber.


The component was placed in the vacuum chamber (0.015 m^3) and the system was then pumped using an KJL Lion 802 (800 l/s) diode ion pump and a Divac diaphragm pump at ambient temperature for 24 hours, after which a background scan and the total pressure in the test chamber were recorded again. If the system pressure was better than 5×10^{-9} mbar, the test specimen was baked at 120 °C for 48 hours. The system was then allowed to cool to ambient temperature before a final mass spectrum and the total pressure in the test chamber were recorded. These final RGA scans are shown below.

NOTE: Exact reproduction of these results should not be expected, as RGA data depends on many factors including environmental factors and initial chamber conditions. However, the data is fully representative of vacuum performance.


TONiC UHV readhead with 1.0 m cable after bake-out (total pressure = 9.0×10^{-10} mbar)

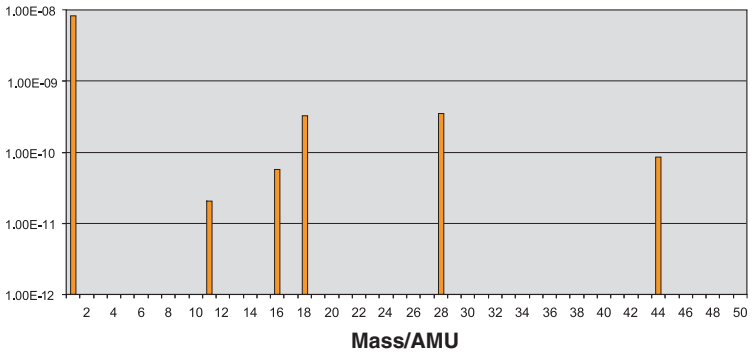

RSLM20 linear scale (180 mm length) with two clips and one clamp after bake-out (total pressure = 3.0×10^{-10} mbar)

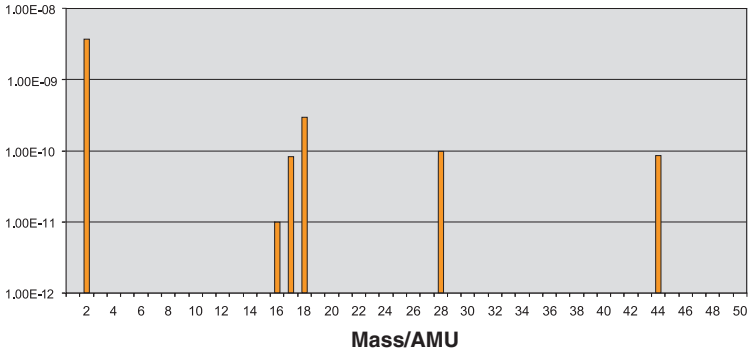


RESM20 (Ø115 mm) after bake-out (total pressure = 7.76×10^{-10} mbar)

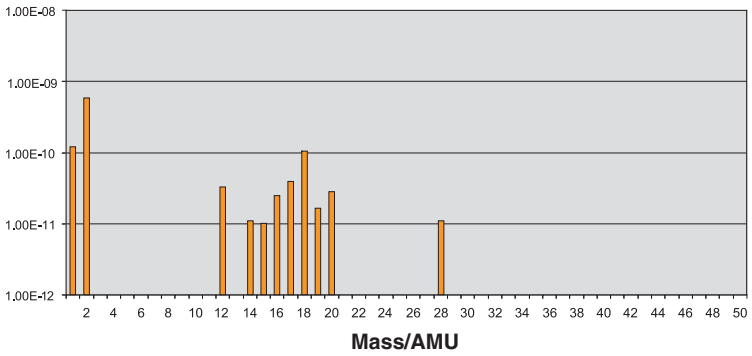

Electrical connections

Grounding and shielding

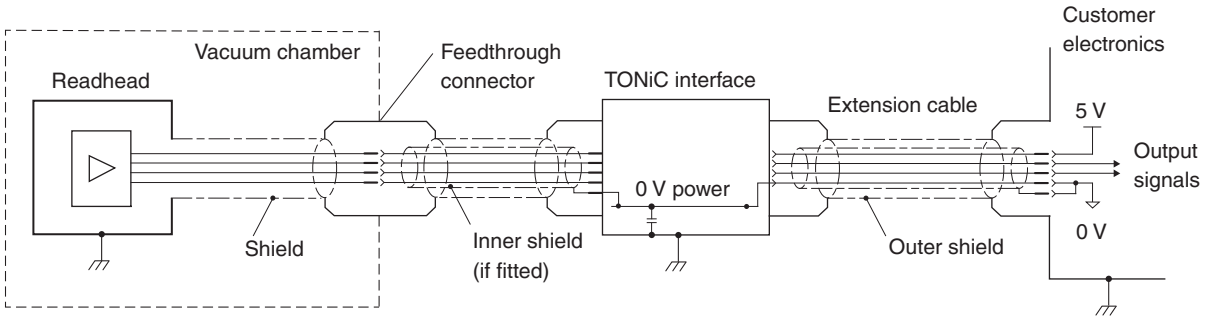

IMPORTANT: The outer shield should be connected to the machine earth (Field Ground). The inner shield should be connected to 0 V at receiving electronics only. Care should be taken to ensure that the inner and outer shields are insulated from each other. If the inner and outer shields are connected together, this will cause a short between 0 V and earth, which could cause electrical noise issues.


Maximum cable length

Readhead to interface: 10 m

Interface to controller: Dependent on clocked output option. See table below for details.

Receiver clock frequency (MHz)	Maximum cable length (m)
40 to 50	25
< 40	50
analogue	50

Remote CAL operation (analogue versions only)




All Ti and TD interfaces include a push-button switch to enable CAL/AGC features.

Remote operation of the CAL/AGC is possible via pin 14 of analogue Ti0000 interfaces.

For applications where no interface is used, remote operation of CAL/AGC is essential.

Recommended signal termination


Digital outputs

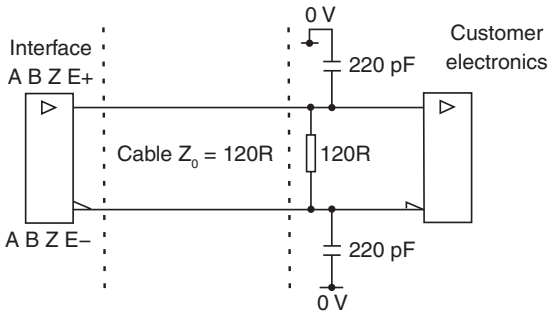


Standard RS422A line receiver circuitry.

Capacitors recommended for improved noise immunity.


Single-ended alarm signal termination (Ti options A, B, C, D)

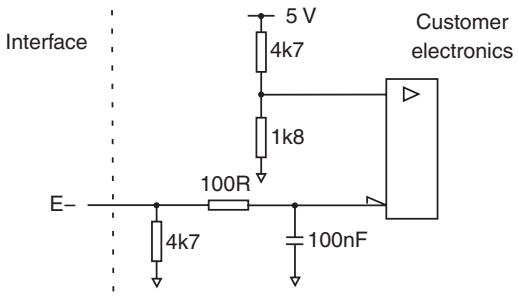

Limit outputs (Ti interface only)



Analogue outputs



[1] Select R so maximum current does not exceed 20 mA. Alternatively, use a suitable relay or opto-isolator.

Output specifications


Digital output signals

Interface models Ti0004 – Ti20KD and TD4000 – TD0040

Form – Square wave differential line driver to EIA RS422A (except limits P and Q).


Incremental [1]

Two channels A and B in quadrature (90° phase shifted)

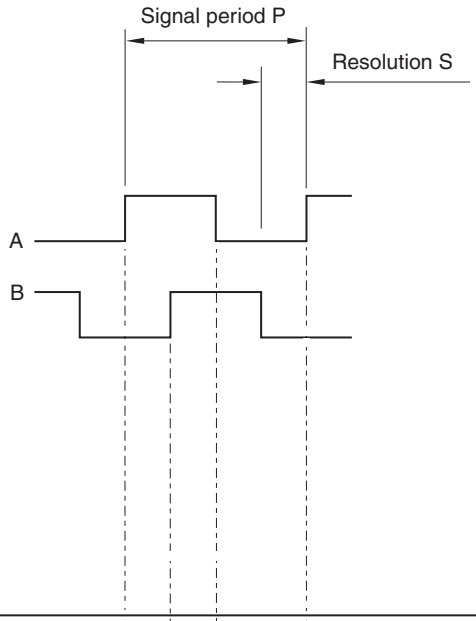

Model	P (µm)	S (µm)
Ti0004	20	5
Ti0020	4	1
Ti0040	2	0.5
Ti0100	0.8	0.2
Ti0200	0.4	0.1
Ti0400	0.2	0.05
Ti1000	0.08	0.02
Ti2000	0.04	0.01
Ti4000	0.02	0.005
Ti10KD	0.008	0.002
Ti20KD	0.004	0.001

Reference [1]



Synchronised pulse Z, duration as resolution.
Bi-directionally repeatable. [2]

Wide reference [1]



Synchronised pulse Z, duration as signal period.
Bi-directionally repeatable. [2]

NOTES:

- Select “standard” or “wide” reference at time of ordering, to match the requirements of the controller being used.
- Wide reference mark not available on Ti0004.


[1] For clarity, the inverse signals are not shown.

[2] Only the calibrated reference mark is bi-directionally repeatable.

Limits

Open collector output, asynchronous pulse.

Digital Ti interfaces only

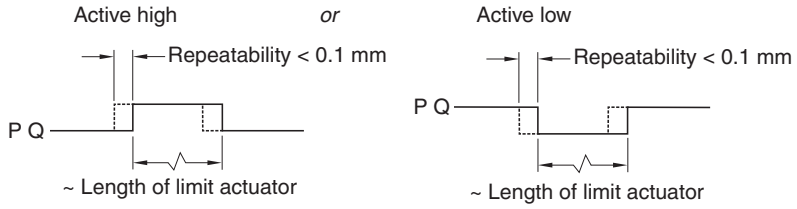


NOTES:

- There are no limits on TD interfaces.
- P limit becomes E+ for Ti options E, F, G and H.

Alarm [1]

Line driven (asynchronous pulse)

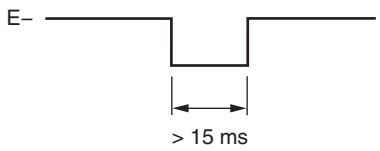


Alarm asserted when:
- Signal amplitude < 20% or > 135%
- Readhead speed too high for reliable operation

Inverse signal E+ only available for Ti options E, F, G and H.

or 3-state alarm

Differentially transmitted signals are forced open circuit for > 15 ms when the alarm conditions are valid.

Set-up [2]

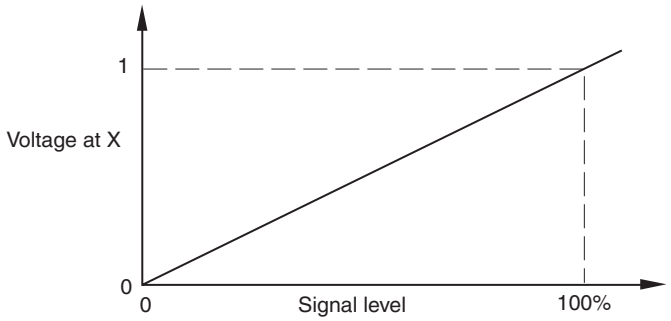

The set-up signal voltage is proportional to incremental signal amplitude.

[1] For clarity, the inverse signals are not shown.


[2] The set-up signal as shown is not present during the calibration routine.

Analogue output signals

Interface model Ti0000 and direct output from all readheads

Incremental


Two channels V_1 and V_2 differential sinusoids in quadrature, centred on 1.65 V (90° phase shifted).

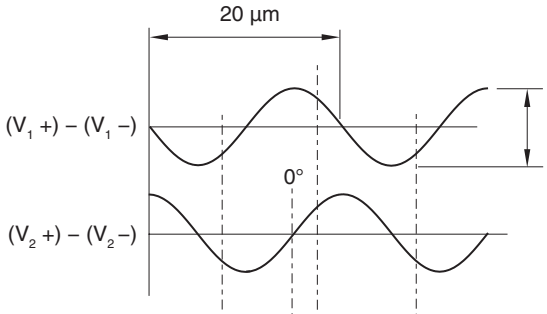

0.7 to 1.35 Vpp with green LED indication (readhead) and 120R termination.

NOTE: Ti0000A00V centred on 2.5 V.

Reference

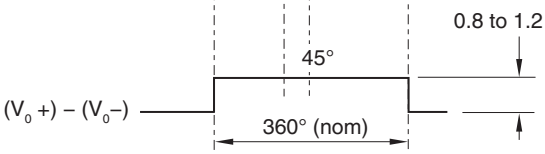

Bi-directionally repeatable. [1]


Differential pulse V_0 centred on 45°.

Limits

Open collector output, asynchronous pulse.


Ti0000 interface only

Active high

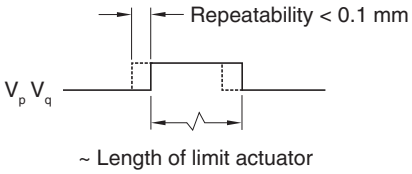


Direct output from readhead

Active low

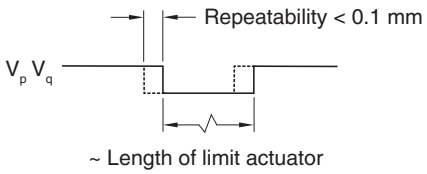

NOTE: Ti0000 interface contains a transistor to invert the readhead's "active low" signal to give an "active high" output.

Set-up [2]

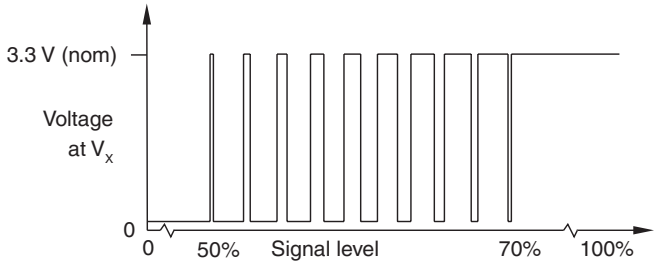

Between 50% and 70% signal level, V_X is a duty cycle.


Time spent at 3.3 V increases with incremental signal level.

At > 70% signal level V_X is nominal 3.3 V.

[1] Only the calibrated reference mark is bi-directionally repeatable.

[2] The set-up signal as shown is not present during calibration routine.


Linear readhead part numbers

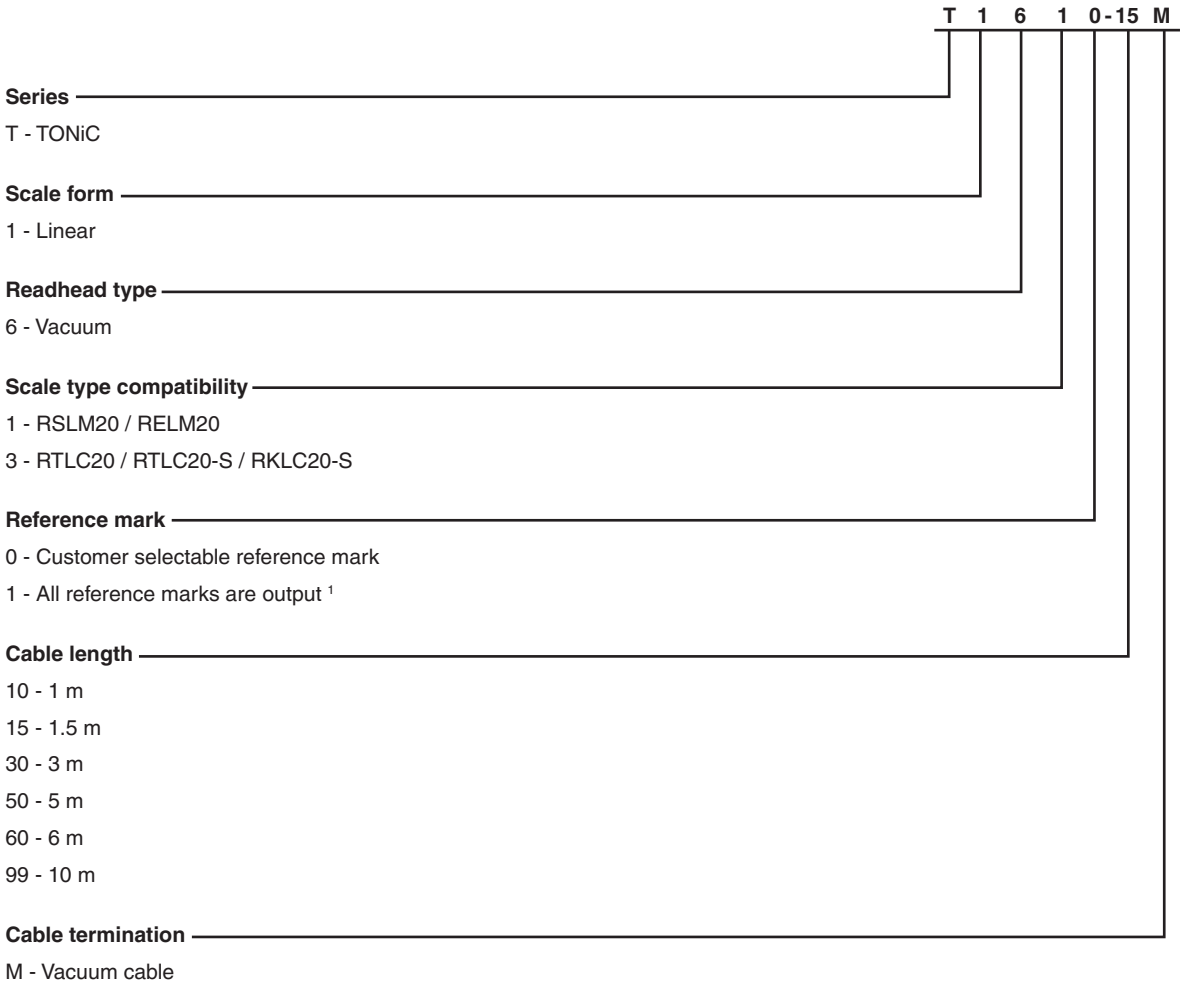

NOTE: Not all combinations are valid. Check valid options online at **www.renishaw.com/epc**.

[1] Only the calibrated reference mark is bi-directionally repeatable.

Rotary readhead part numbers

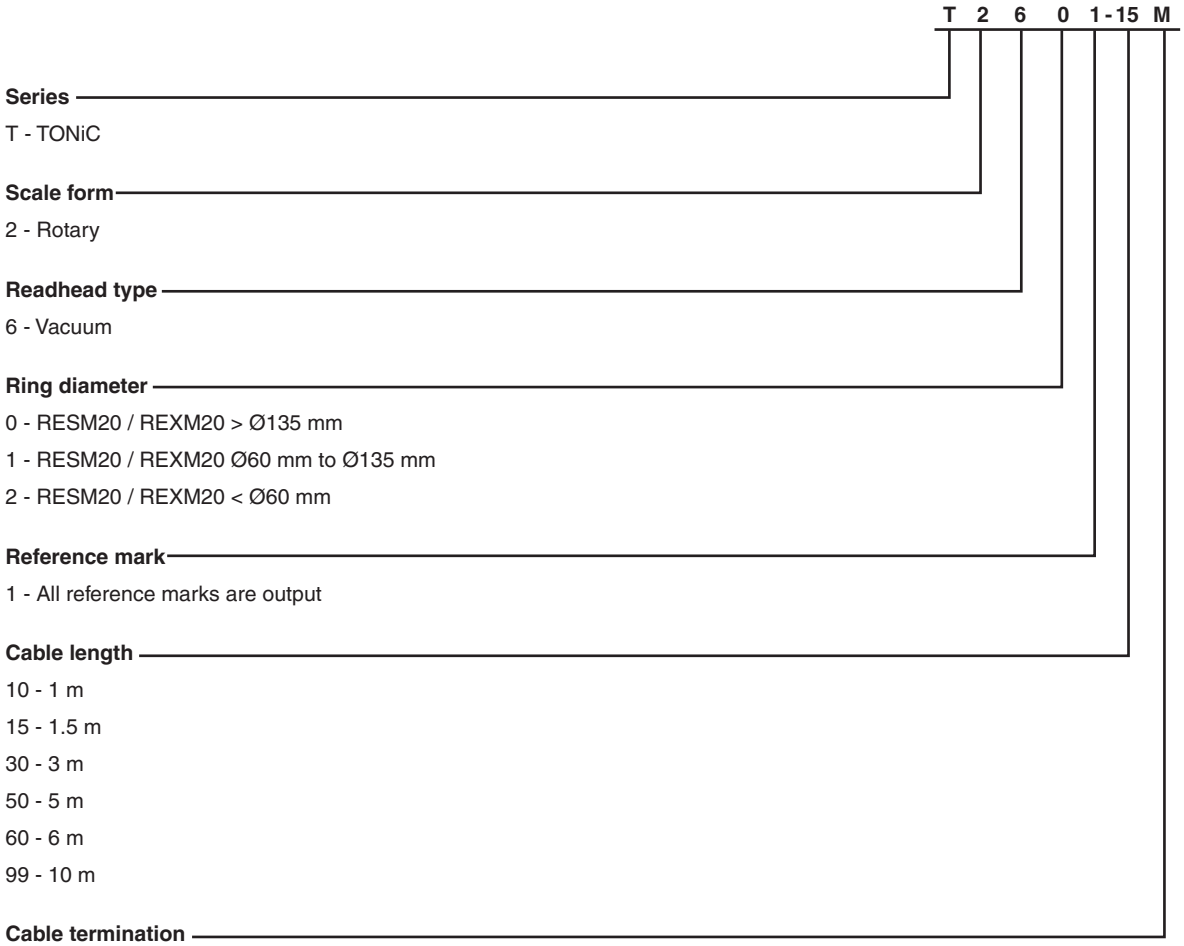

NOTES:

- Not all combinations are valid. Check valid options online at **www.renishaw.com/epc**.
- Contact your local Renishaw representative if you require a partial arc application.

Ti interface part numbers

Compatible with all TONiC readheads

Analogue

Ti 0000 A 00 A

Options

A - Dual active high limits

V - 2V5 Vmid dual active high limits

Digital

Ti 0200 A 20 A

Series

Ti - TONiC interface

Interpolation factor/resolution [1]

0004 - 5 µm [2]	1000 - 20 nm
0020 - 1 µm	2000 - 10 nm
0040 - 0.5 µm	4000 - 5 nm
0100 - 0.2 µm	10KD - 2 nm
0200 - 0.1 µm	20KD - 1 nm
0400 - 50 nm	

Alarm format and conditions [3]

A - Line driven E output; All alarms

B - Line driven E output; Low signal and high signal alarms only

E - 3-state; All alarms

F - 3-state; Low signal and high signal alarms only

Clocked output option [3]

50 - 50 MHz	10 - 10 MHz
40 - 40 MHz	08 - 8 MHz
25 - 25 MHz	06 - 6 MHz
20 - 20 MHz	04 - 4 MHz
12 - 12 MHz	01 - 1 MHz

Options

A - P/Q limits – “active high”, standard reference mark

B - P/Q limits – “active low”, standard reference mark

C - P/Q limits – “active high”, wide reference mark [2]

D - P/Q limits – “active low”, wide reference mark [2]

E - Q limit only – “active high”, differential alarm, standard reference mark

F - Q limit only – “active low”, differential alarm, standard reference mark

G - Q limit only – “active high”, differential alarm, wide reference mark [2]

H - Q limit only – “active low”, differential alarm, wide reference mark [2]

NOTES:

- Only the readhead is UHV compatible; the Ti interface must be kept outside the vacuum chamber.
- Not all combinations are valid. Check valid options online at www.renishaw.com/epc.

[1] Additional interpolation factors available. Contact your local Renishaw representative for further details.

[2] Wide reference mark not available on Ti0004 (5 µm) interfaces.

[3] When using with a DSi, the interface should be configured with line-driven alarm outputs and a clocked output option of 01, 04, 06, 08, 10, 12 or 20.

TD interface part numbers

Compatible with all TONiC readheads

Dual resolution

TD 4000 A 20 A

Series

TD - TONiC dual resolution

Interpolation factor/resolution [1]

Pin 10 open	Pin 10 = 0 V
4000 - 5 nm	10 nm
2000 - 10 nm	20 nm
1000 - 20 nm	40 nm
0400 - 50 nm	0.1 µm
0200 - 0.1 µm	0.2 µm
0040 - 0.5 µm	1 µm

Alarm format and conditions [2]

A - Line driven, differential output; All alarms

B - Line driven, differential output; Low signal and high signal alarms only

E - 3-state; All alarms

F - 3-state; Low signal and high signal alarms only

Clocked output option [2]

50 - 50 MHz	10 - 10 MHz
40 - 40 MHz	08 - 8 MHz
25 - 25 MHz	06 - 6 MHz
20 - 20 MHz	04 - 4 MHz
12 - 12 MHz	01 - 1 MHz

Options

A - Standard reference mark

B - Wide reference mark

NOTES:

- Only the readhead is UHV compatible; the TD interface must be kept outside the vacuum chamber.
- Not all combinations are valid. Check valid options online at **www.renishaw.com/epc**.


[1] Additional interpolation factors are available. Contact your local Renishaw representative for further details.

[2] When using with a DSi, the interface should be configured with line-driven alarm outputs and a clocked output option of 01, 04, 06, 08, 10, 12 or 20.






RENISHAW
apply innovation™

TONiC UHV compatible products




TONiC series

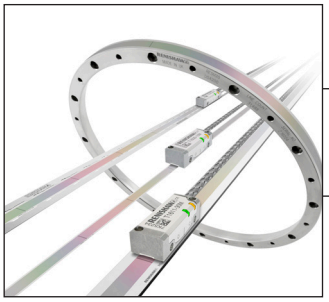

T16xx

-  RTLC20-S self-adhesive tape scale
-  RTLC20 tape scale and FASTRACK carrier
-  RKLC20-S self-adhesive mastered tape scale
-  RELM20 self-adhesive or clip/clamp mounted ZeroMet spar scale
-  RSLM20 self-adhesive or clip/clamp mounted stainless steel spar scale

T26xx

-  RESM20 stainless-steel ring
-  REXM20 high-accuracy stainless-steel ring
-  DSi for dual-readhead rotary systems

www.renishaw.com/contact

#renishaw

+44 (0) 1453 524524 **uk@renishaw.com**

© 2009–2026 Renishaw plc. All rights reserved. This document may not be copied or reproduced in whole or in part, or transferred to any other media or language by any means, without the prior written permission of Renishaw.
RENISHAW® and the probe symbol are registered trade marks of Renishaw plc. Renishaw product names, designations and the mark "apply innovation" are trade marks of Renishaw plc or its subsidiaries. Other brand, product or company names are trade marks of their respective owners.
WHILE CONSIDERABLE EFFORT WAS MADE TO VERIFY THE ACCURACY OF THIS DOCUMENT AT PUBLICATION, ALL WARRANTIES, CONDITIONS, REPRESENTATIONS AND LIABILITY, HOWSOEVER ARISING, ARE EXCLUDED TO THE EXTENT PERMITTED BY LAW.
RENISHAW RESERVES THE RIGHT TO MAKE CHANGES TO THIS DOCUMENT AND TO THE EQUIPMENT, AND/OR SOFTWARE AND THE SPECIFICATION DESCRIBED HEREIN WITHOUT OBLIGATION TO PROVIDE NOTICE OF SUCH CHANGES.
Renishaw plc. Registered in England and Wales. Company no: 1106260. Registered office: New Mills, Wotton-under-Edge, Glos, GL12 8JR, UK.

Part no.: L-9517-9426-04-B
Issued: 11.2026